



# Hypertronic Pro

## Operating Guide

6 August 2018

[www.hypertronicpro.com](http://www.hypertronicpro.com)

Congratulations on choosing to purchase the Hypertronic Pro. By doing so you now have the assurance and peace of mind that comes with purchasing a device built and tuned to the highest quality and performance standards, and backed by a comprehensive 1-year warranty. We hope you enjoy using the Photon Sound Beam Complete for many years to come.

*Warning*

Do not use the Hypertronic Pro until you have read this operating guide from cover to cover.

*Please check for updates to this manual on a regular basis by visiting [www.hypertronicpro.com](http://www.hypertronicpro.com)*

# CONTENTS

1. Introduction
2. The Hypertronic Pro in Detail
3. Procedures
  - a. Switching on and Preparing the Hypertronic Pro for Use
  - b. Broadcasting and Making Remedies
  - c. Creating Vibrational Remedies
  - d. Copying Vibrational Remedies
4. Useful Radionic Rates Guides for Users of the Hypertronic Pro (Free to download)
5. Cleaning and Caring for your Hypertronic Pro
6. Warranty
7. Disclaimer

# 1. INTRODUCTION

*RADIONICS at its best ....*

Achieve good health physically, emotionally and mentally through use of this simple to use radionics system. Broadcast healing energies or psychometry with no limitation on distance, or make vibrational medicine remedies in an instant. Little to no training required in use of this scientific instrument.

Suitable for both Professionals or the Home User.

## FEATURES OF THE HYPERTRONIC PRO INCLUDE THE ABILITY TO;



- assess biological sample and to apply a mirror frequency to rectify bodily energies for better health. Biological samples can be applied in the form of
  - a drop of blood,
  - hair
  - a photo (real or digital)
  - voice recording (the unit features a microphone for this assessment)
- create and duplicate any homoeopathic remedy (electronic homoeopathy)
- apply healing radionic rates for broadcast or vibrational medicine remedies (in the form of drops or pillules)
- create vibrational medicine remedies or broadcast healing frequencies to any subject anywhere in the world
- apply psychometry to any subject locally or from afar

### **Optional**

- connect the Hypertronic Pro to your computer and use the software Rife Pro X2 to include powerful Rife Frequencies and Hulda Clarke frequencies in your energy medicine formula
- integrate with the Photon Sound Beam to broadcast healing frequencies



## 2. THE HYPERTRONIC PRO IN DETAIL

The Hypertronic Pro is a state-of-the-art scientific instrument, that provides a quantum leap in balancing overall health of the natural energy fields in the body.

The Hypertronic Pro is designed to measure and balance what are known as intrinsic data fields (IDFs). Intrinsic data fields are believed to be subtle informational fields which surround all living and non living material things in nature. They are believed to be part of the morphogenetic field theorized by Rupert Sheldrake. The Hypertronic Pro represents a significant advance in design, from models on which it is based including the BioMirror and other non computer based radionics systems.

Unlike the advanced Radionics Systems that use a traditional approach of using analytical software that place a disease label on symptoms present in a patient, the Hypertronic Pro takes a more modern approach, disregarding symptoms and disease labels, and looks at intrinsic data field frequencies representing disharmony from the entire individual. It then mirrors the inverse frequency of the intrinsic data fields to create a balancing and healing effect on the body. Healing frequencies are delivered either by broadcast (where there is no limitation on distance between machine and patient), or by remedy, which can be made by the Hypertronic Pro in a small dropper bottle consisting of pure water, and 25% brandy as a preservative. Once harmony is restored to the body energetically, then it is up to the body to use these frequency adjustments for natural healing.

### **Why the name "Hypertronic Pro"?**

The Hypertronic Pro is so named as it uses HYPERspace (or theoretical dimensions defined in string theory physics and mathematics) to deliver healing energies electRONICally. The theoretical basis to radionics lies in dimensions beyond our 4 dimensions, as explained in Scientific Theories of Radionics. This instrument can be used by home users in its most basic mirroring mode, or by advanced trained PRO users in an advanced clinical setting using homoeopathy or other vibrational medicine therapies to treat patients on a day to day basis.

The Hypertronic Pro is an advanced design on the original Jeff Byrd 97 BioMirror, and 2 other contemporary radionic instruments. The BioMirror was a unit designed in the early 2000s which was rated as one of the top radionics instruments in the world by a leading Canadian psychotronic practitioner, namely James Black. The Hypertronic Pro uses the same circuitry as the deprecated BioMirror. It has all the features for someone adept at radionics and for someone just starting out. It is different in appearance from a traditional radionic instrument which has many knobs crowding the console of the instrument, whereas the Hypertronic Pro has a compact array of rate selectors (marked Code) simulating a traditional 12 stage radionic instrument.

A new generation of psychotronics, Hypertronic Pro is a powerful, Holographic Scalar Energy Broadcasting instrument utilizing biological samples for holographic vibrational energy transfer. At last we have choices in maintaining perfect health that is quick, easy and affordable, and now with the convenience of Remote Broadcasting at a distance.



The Hypertronic Pro combines a number of the top professional radionic modalities into the one instrument;

- The Hypertronic Pro allows assessment of incoherent bodily frequencies from a modern holistic viewpoint, disregarding the step of complex analysis which puts symptoms into a disease label. It then uses this information to reverse the disharmony energetics to encourage healing.
- The Hypertronic Pro allows remedies to be made in the form of

homeopathic remedies and vibrational essences using radionic rates available in free [downloadable guidebooks](#).

- The Hypertronic Pro allows broadcasting of healing frequencies with no limit on distance between the Hypertronic Pro and the client.
- The Hypertronic Pro allows the option of copying vibrational medicine remedies.
- There is an input port built into the Hypertronic Pro, specially designed to allow a connection with the Photon Sound Beam. This allows the broadcast facility in the Hypertronic Pro to send Photon Sound Beam healing frequencies to afar.

### **Vibrational Medicine Remedies that can be Electronically Made**

Using the Hypertronic Pro, there is no limit to vibrational remedies that can be made using rates from the free downloadable guidebooks. Examples of remedies that can be made include;

- Homoeopathic Remedies (for treatment of chronic and acute illness etc)
- Flower Essence Remedies (for treatment of emotional conditions) including Bach Flower Remedies, Australian Bush Flower Essence Remedies, Bailey Flower Essences, Californian Flower Essences and the Gurudas Flower Essences
- Homoeopathic Vaccines
- Acupuncture Meridian Remedies
- Allergy Remedies
- Parasite Remedies

To make a remedy, place a small dropper bottle with 75% water and 25% brandy (used as a preservative) onto the right hand plate. Consult the guidebook and dial the rate (and potency for homoeopathics) into the Hypertronic Pro and then expose the remedy to the frequency. You now have a remedy that can be used normally by taking several drops under the tongue, and then holding the drops there for a minute or so before swallowing.

In addition to being able to make remedies using radionic rates, the Hypertronic Pro gives the user the option to copy vibrational remedies by placing a remedy onto the left witness plate, then a blank remedy onto the right broadcast plate, and exposing the blank remedy to the frequencies of the remedy being copied.

*Hypertronic Pro features include;*


- Voice Potentizer. You can record the clients voice, and the measurements can be made using the recording rather than a biological sample.
- Holographic Scalar Energy Witness Broadcasting (Achieved through utilizing biological samples for holographic vibrational energy transfer).
- Radionics rates for free download.
- Vibrational remedy transfer from left plate to right plate.
- Diagnostic touch-plate (Stick plate) with twin dials (useful for psychometry).
- Extraneous noise filtration to remove all frequencies from outside of the witness sample and broadcast plate. Earlier versions of the Hypertronic Pro had issues where power signal was noisy which affected the sample, but this issue has now been resolved in the Hypertronic Pro.
- Option for including radio frequency (RF) input such as the output frequencies of Photon Sound Beam for broadcast (see photon sound beam integration below).
- Optional full-spectrum (thought to light frequencies) holistic Holographic Broadcasting (for psychometry work).
- Input and output connectors for external use.
- A copper rod for direct delivery of energies to the patient through the output port.
- A copper board plate with extension cord for witness samples too large for the left plate on the Hypertronic Pro.
- Controls for Power, Homoeopathic Potencies, Continuous use, Clearing the system for new client, Energizing remedies, Codes and more.
- Comes with a 12V power supply which uses 110-240V electrical feed (suitable for use in any country).
- Operating Manual



### **Integration with Rife Pro X2 Software and your Computer (Optional)**

You can optionally purchase the Rife Pro X2 computer software, which can be used with the Hypertronic Pro. Using the Rife Pro software, you are effectively turning your computer into a Rife



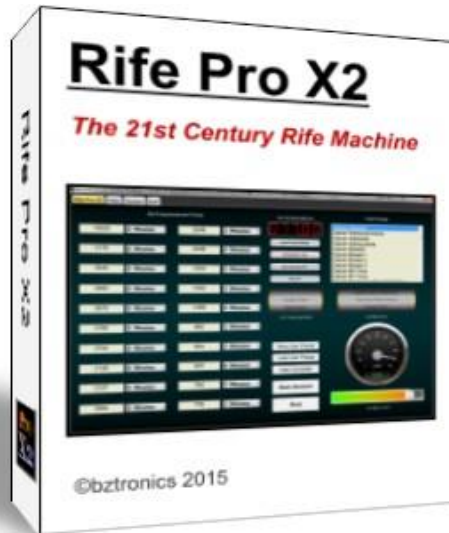

machine. Instead of delivering the Rife frequencies in the form of sound, the frequencies are fed directly into the Hypertronic Pro circuit, allowing you to make remedies or to create a targeted broadcast based on biological matter on the witness plate.

Imagine helping a relative with insomnia that lives far away, or a friend with a health disorder. Simply ask them for a hair sample, and you are ready to treat them using the Rife Pro and the broadcast on the Hypertronic Pro.

Rife Pro X2 is the latest Rife Technology. It has a powerful Rife Frequency Generation system that lets you use your computer as a Rife Machine.

It's more versatile than any other Rife Machine, because it also lets you structure water and oils with frequencies - so you can make homeopathic remedies. It also has a built-in TBSW system for pain relief, insomnia, weight loss and more.

Rife Pro X2 is easy for anyone to use - no complicated scripts and programming required as with other Rife Machines. All it takes is a couple of mouse clicks and you're up and running. There's no need for a bunch of clunky wires and electrodes either. Special algorithms in the software let you use speakers or headphones to deliver Rife frequencies, safely and naturally (explained later).

You'll see real results with Rife Pro X2, even when drugs and other methods have entirely failed. If you really want to get rid of something - you need to get to the "source" of the problem. That's what Rife Pro X2 does. It gets directly to the source of the problems.



### **Photon Sound Beam Integration (Optional)**


The Hypertronic Pro can be used completely independently by itself, or synergistically for enhanced results with the Photon Sound Beam. Both the Hypertronic Pro and



Photon Sound Beam are engineered and manufactured by the same development team. There is a specially designed port in the Hypertronic Pro which allows the RFSP port on the Photon Sound Beam to directly connect to the Hypertronic Pro. This can be used for the following options;

Allow the Hypertronic Pro to broadcast Photon Sound Beam frequencies (e.g., the general sweep on the level 12 setting for 30 mins) to any patient (with their permission) using their biological sample, voice print or picture worldwide.

When using the Photon Sound Beam for a therapy session, allows the Hypertronic Pro to send inverse mirrored energies back to the Photon Sound Beam for inclusion in the hand held plasma tubes.

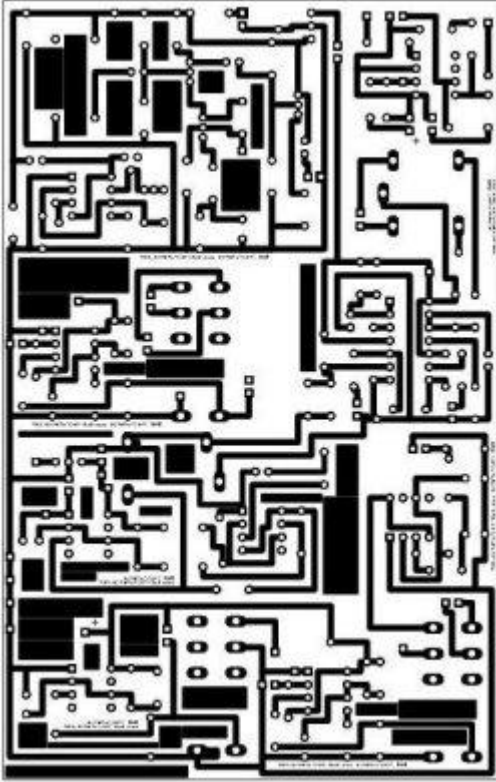

## How Hypertronic Pro Works

The Hypertronic Pro has 2 primary systems;

1. A BioMirror where intrinsic data fields are measured in the form of a frequency pattern, and the reverse of this pattern is applied back to the patient to create an energy correction, which in turn allows physical correction (healing) to follow.
2. A Powered Radionics System which may be regarded as an electronic extension of a person's intention (belief helps to provide mental structure to it). The Hypertronic Pro is a standard Radionic instrument that links the mind with the primal or causal levels of creation and manifestation. These are variously referred to as the Morphogenetic Field, Holographic Fields, Hyper-Space, Scalar Energies and so forth.

The Hypertronic Pro utilizes a harmonically-rich, pure square-wave electromagnetic field through which a biological sample (e.g., blood, urine, hair, or fingernails)

are broadcast with exclusively designed transfer plates. The Hypertronic Pro is also capable of achieving this through use of a photo or voice imprint of the patient.

Underneath the output plate there are several electronic parts including a specially designed swirl symbol which is sacred geometric compliant, as well as a harmonics speaker allowing rich delivery of multiple signals. There are no inline orgonite or pyramid structures included in the Hypertronic Pro. Some other radionics machines use such parts, but they are regarded by the developers of Hypertronic Pro as a non requirement. It should be duly noted that parts such as orgonite components can in fact be damaging as energies that are emitted are often misaligned with bodily harmonics and can thereby stress bodily organs and lead to longer term health issues.

## Inputs and Outputs on the Rear of the Hypertronic Pro

The Hypertronic Pro has 5 connector plugs on the rear of the unit as shown in the following photo.



Labels have been placed on the photo to identify each of the connectors, as follows;


- **A** The black banana jack is for the large extension witness plate, which is used when the left hand witness plate on the unit is too small.
- **B** This is a 3.5 mm stereo input jack, which is used for the optional Photon Sound Beam connection to send RF from the RFSP port of the Photon Sound Beam to the Hypertronic Pro. It can optionally be used to include any length of audio input (e.g., a 30 min monologue while the unit is in continuous mode, or healing frequencies from tuning forks etc) from another unit such as a computer sound card, computer headphone outlet, an iPod, iPhone, mp3 player, radio or any other device that has *standard line level audio output* (Note: Standard Line Level Output is usually audio output suitable for headphones and must not exceed 1V RMS which can otherwise void warranty on the Hypertronic Pro. It is recommended that you check audio output specifications for the unit you are attaching *before* connecting).
- **C** This is where the power lead is connected.
- **D** This is a 3.5mm connector plug, used to connect to frequencies from the Hypertronic Pro back into the Photon Sound Beam via the RFSP port.
- **E** Is the banana jack output connector, allowing you to connect the copper handle for the patient to hold, for a direct treatment.

## Other Features

- **Potency:** This feature allows one to select the strength at which the subtle energies are sent to the "OUT" Plate. Set the knob to "0" for a generic general broadcast.

- **Transfer Only/Continuous Switch:** This allows the user to use either a standard timed energy transfer to the out plate, or to engage in a Continuous transfer to the out plate. It is usually recommended that you use the Transfer Only mode.

- **Harmonics Switch:** There are 3 positions including Fast, None (center), and Slow. Harmonics can be included in timed OR continuous cycles. Previously models on which this design is based had it that

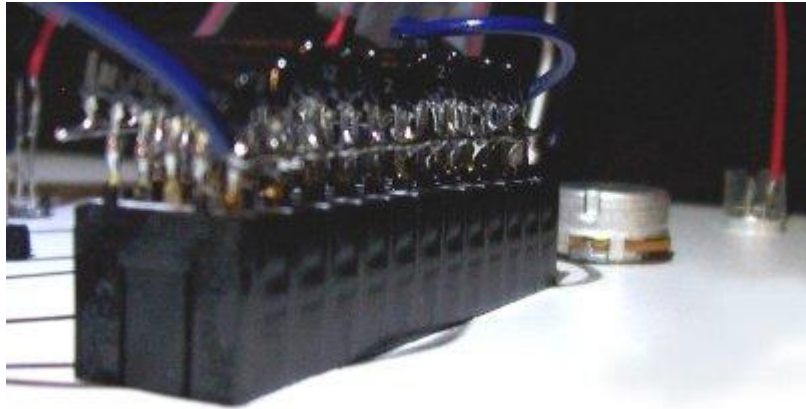

harmonics could only in included in the continuous cycle but this limitation has been removed in the Hypertronic Pro.

a. No Output -- MIDDLE POSITION

b. In FAST or SLOW position -- simply ADDS RF Harmonics to the broadcast e.g., 10MHz which penetrate the body easily as carry wave, 15Hz which is energetic, as well as 10Hz, 27Hz and 40MHz. All good for carrying required healing frequencies into the body.

- **"Rates"** Control Switch: Enter a Radionic Rate (analogous to frequency) from the Rate Listing provided. CopenLabs Rates Book may be downloaded from [hypertronicpro.com](http://hypertronicpro.com).
- The **IMPRINT RATES** below the "Potency" is used if desired to ADD a specified number for the selected Homeopathic "Potency" such as 30x or 100c potency.
- **Body:** this optional feature selects the chakra level at which you wish to direct the broadcast, such as "1" for more gross physical application (or root chakra) or "7" for the most subtle (or crown chakra). When not using this feature, set to "0".
- **Record/Playback:** This setting functions as a *Voice Potentizer*. A voice recording of one's own voice vibration (or the client's) or other recording may be used to overlay the subtle energy broadcast. Use: While holding down the *Record* toggle switch, place a recording or speak clearly and loudly as near a possible into the black foam covered microphone. There is a 20 second maximum recording time. The *Playback* toggle selection may be used to confirm a recording. The volume is not a factor in results and is intentionally very low for a clean subtle energy signal. *Note:* Pressing the *Record* toggle once will erase the previous recording. The *Clear* button or powering down does not erase the recording.
- **Rub Plate:** (Lower right-hand corner) This is an optional tool for connecting operator mind and for tuning thoughts with reality for finer radionic adjustment. By gently stroking the surface of the small plate with a finger(s) (usually in direction towards the user) a change in the energy

level can be felt on finger tips with a "sticking effect". The 2 knobs are adjusted accordingly to fine tune the broadcast plate with intention and manifestation when needed.

### **Electronic Specifications**

Prior to mid-July 2017, the Hypertronic Pro used electronic parts with a unity level of 300MHz. These parts are still capable of handling frequencies exceeding 500MHz, but just not as effectively as 300MHz and below. From mid-July 2017, the Hypertronic Pro was built with high end specification electronic parts, which are capable of handling frequencies as high as 1.1GHz. Many other competitive radionic machines are limited by the electronic part specifications which they use, and are therefore less effective on this note alone when compared with the Hypertronic Pro.

# 3. PROCEDURES

## 3a. SWITCHING ON AND PREPARING THE HYPERTRONIC PRO FOR USE

This instrument is designed to be used in a holistic holographic broadcast-mode where all the subtle energy rates are broadcasted simultaneously. Optionally, one may use rates by referencing a Radionics Rate Book and then broadcast the healing frequency remotely using a biological sample, or there is the alternative of making a vibrational remedy.


### Plugging the Hypertronic Pro into the Power Supply

Plug the 110/240V 12Volt Wall Plug Adapter into a wall socket and the other end into the rear of the Hypertronic Pro into the jack marked C on the rear of the unit (see picture below)



## Turning on and clearing the instrument

Before switching on the Hypertronic Pro, ensure that all knobs, imprint and broadcast rates are set to zero as shown below, to minimize the possibility of interference.

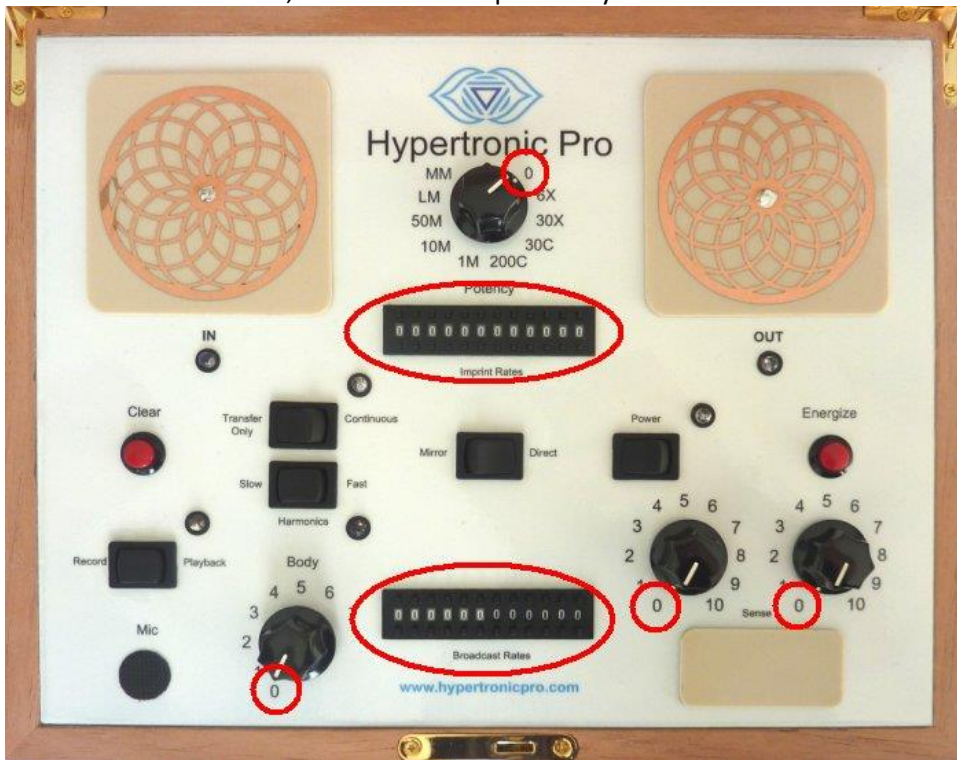


Make sure that the Transfer Only/Continuous Switch is set to TRANSFER ONLY to prevent any immediate broadcast when powering on (which occurs when switched to Continuous).



Press the "Power" toggle switch ON.



Wait for the unit to complete 15 second timed clearing process. The IN and OUT lights will glow red while this process is taking place. Wait until both LEDs have stopped glowing (the IN LED will stop glowing first, followed by the OUT LED).

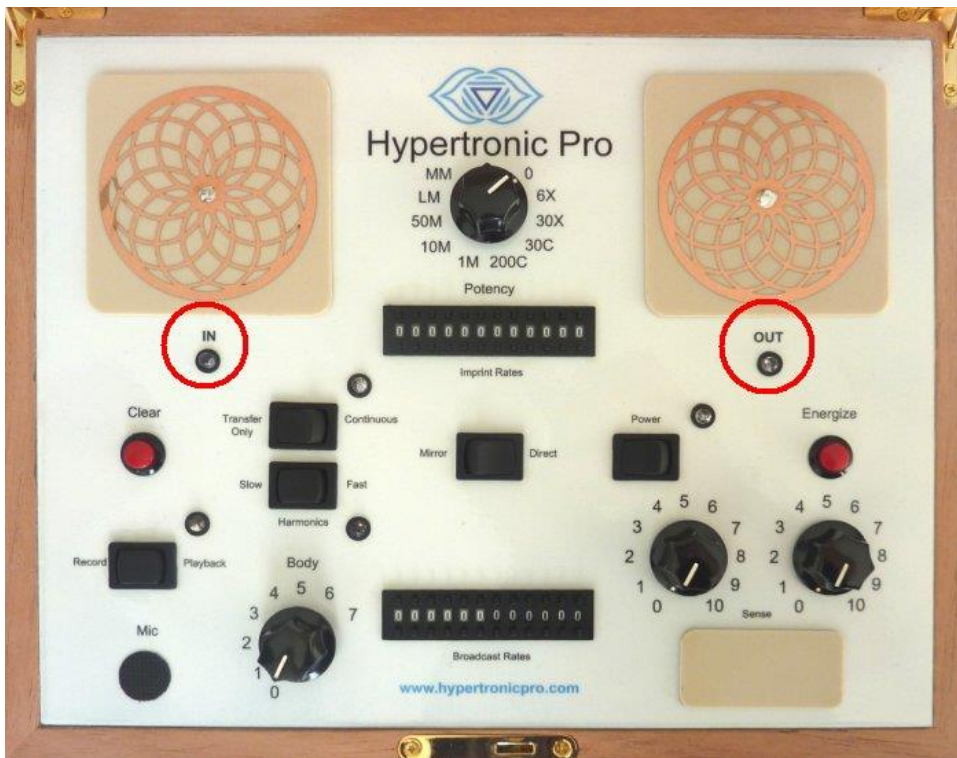



Briefly tap the Record button to remove any recording from the unit's memory.



If the Hypertronic Pro is already switched on, and you need to clear the unit ready for the next patient, reset everything back to zero as described above, clear the witness plate of any biological materials, and then press the Clear button and wait for the 15 second electronic clearing process to complete.



### 3b. BROADCASTING AND MAKING REMEDIES

- After preparing the witness and clearing the machine, place the WITNESS SAMPLE on the left witness plate.




- **Professionals:** Select **Direct** or **Mirror** using the toggle switch shown below.



The **Direct** Selection is used for Making Vibrational Remedies OR Witness Sample Broadcasting when using "RATES".

**Mirror** is used for broadcasting the remedial BioMirror broadcast frequency (see image to right) which is measured from the biological or voice witness sample. The "Mirror" Selection INVERTS the

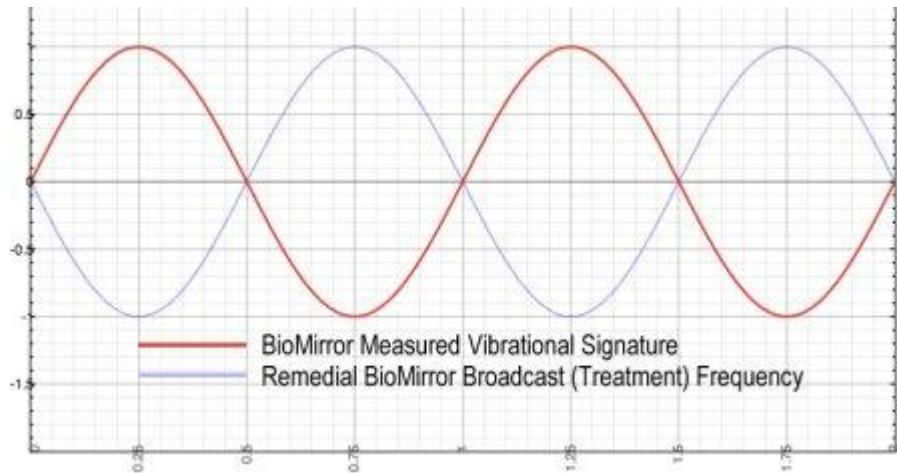

"vibrational signature" of the WITNESS SAMPLE on the In-Plate and Out-Plate EMPTY. Most users primarily use this mode. "Mirror" is a Holistic Holographic Broadcast when one is NOT using "RATES". You may choose to surround the Witness Sample with favorite supplements or remedies to include in the witness.


The Hypertronic Pro can broadcast a treatment to a client located anywhere in the world. It is not necessary for the client to be present when broadcasting.

### Home Users

Select Mirror Switch. Mirror is for broadcasting remedial BioMirror broadcast frequency (see above image). The Hypertronic Pro can broadcast a treatment to a client located anywhere in the world. It is not necessary for the client to be present when broadcasting. Note: The "Mirror" Selection INVERTS the "vibrational signature" of the WITNESS SAMPLE on the In-Plate and Out-Plate EMPTY. Most users primarily use this mode. You may choose to surround the Witness Sample with favorite supplements or remedies to include in the witness.


- **Home Users**

Leave all optional settings at zero or neutral.

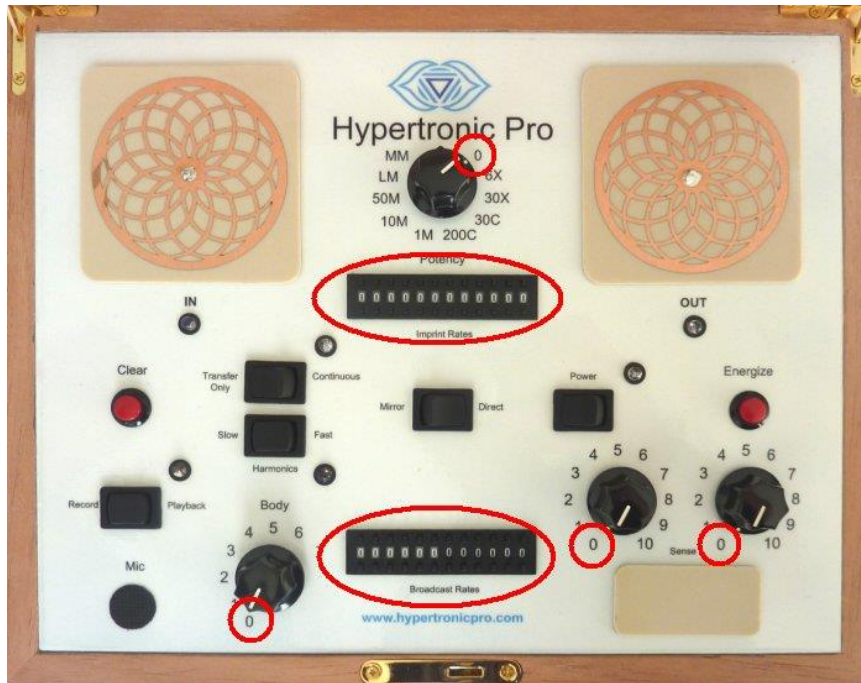

**Professionals**

Optional settings (leave optional settings at zero or neutral if not being used)

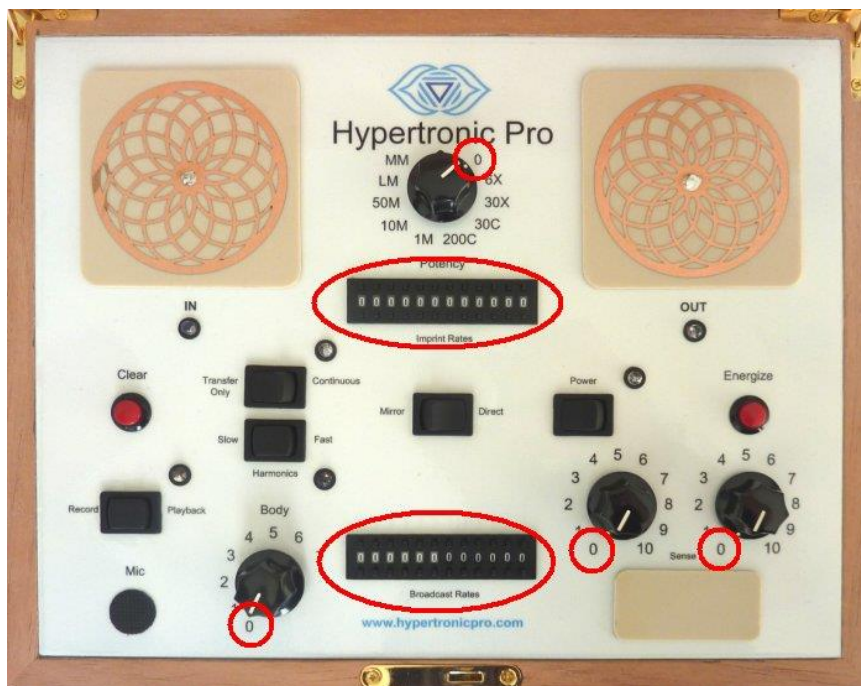


a. Set to HARMONICS, if desired. Slow or fast. Slow is 10MHz, fast is 10MHz pulsed at 15Hz. If you do not want to include harmonics, leave the switch in the middle position which excludes harmonics from the energy cycle. Including harmonics in the cycle simply adds Radio Frequency Harmonics to the broadcast e.g., 10MHz **which penetrates the body easily as carry wave**. Both options are good for carrying required healing frequencies deep into the body.



b. As a general rule, when entering a single number rate for homeopathic remedies, use Imprint Rates.




When broadcasting or needing to mirror, use Broadcast Rates. Broadcast Rates is more for the radionics side of things.

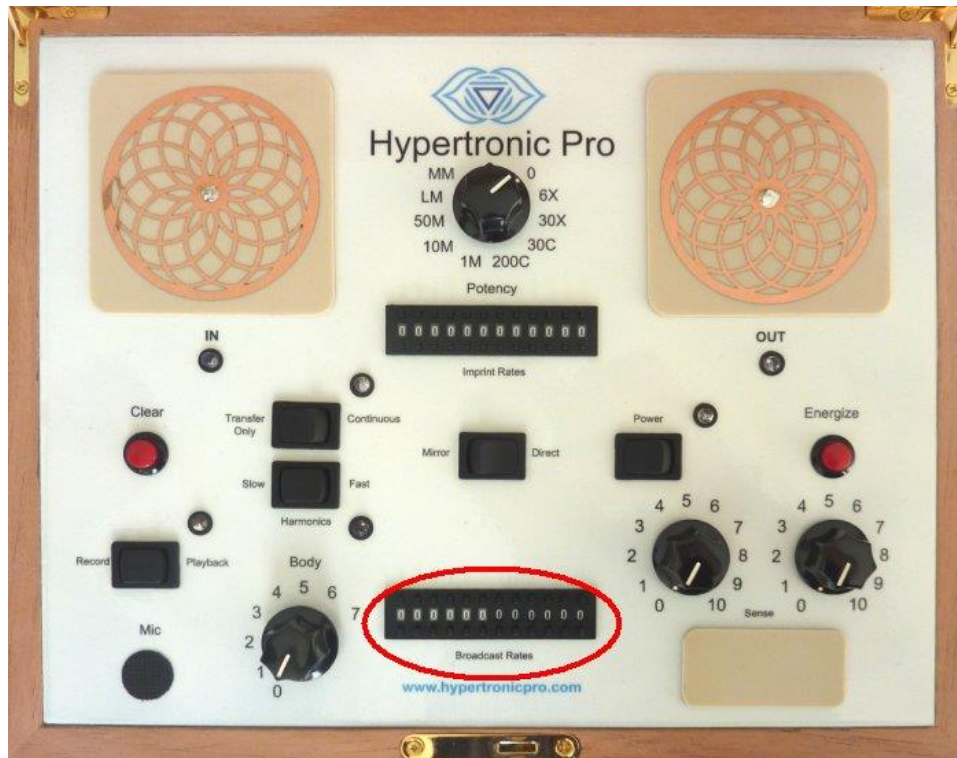

The Voice Playback and Harmonics can still be added to either Imprint Rates or Broadcast Rates. You can input a radionic rate at the lower rate bank: BROADCAST RATES (see above picture).

Rates are found by referencing the [Radionic Guides](#) on our web site (see section 4 in this manual for details). They are [free to download](#) and to use as a reference.


Always make sure numbers are entered from the right side. For example the Sulis guide says that the rate for producing a Typhoid vaccine is 61189991. It should be entered as 000061189991 as shown in the picture below and NOT as 611899910000.

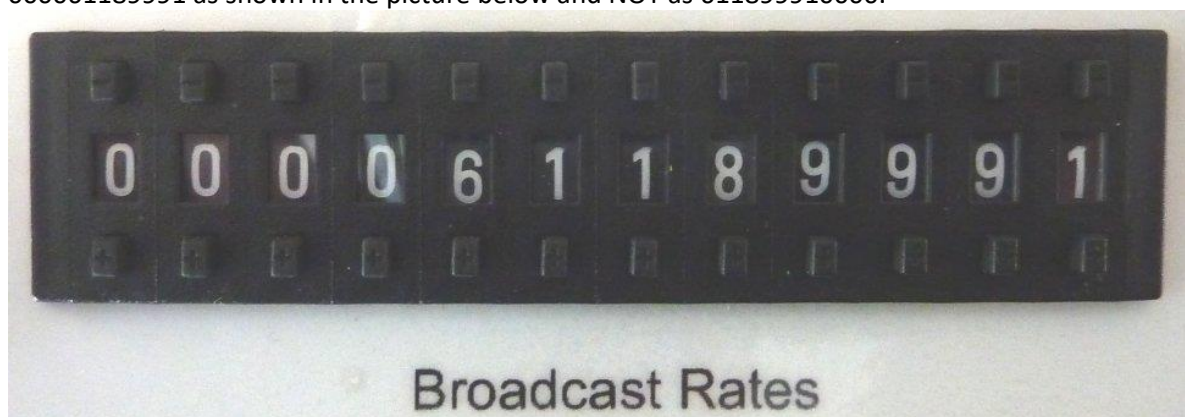

Input a second rate if so desired in the upper bank marked IMPRINT RATES (the second rate cannot be used in MIRROR mode). Most references do however only have the one rate. If by chance you are using the [Kelly Reference for Radionic Rates](#) which consists of 2 rates, the first would go into BROADCAST RATES and the second into IMPRINT RATES. As an example if in the [Kelly Reference Guide](#) we have *left* 31.75 and *right* 23.00, then you would add

00000003175 into BROADCAST RATES and 00000002300 into IMPRINT RATES.

There are buttons above and below each of the numbers in the dial banks. To increase a number by 1, press the button underneath the number (marked + in the picture below). To decrease a number by 1, press the button above the number (marked - in the picture below).

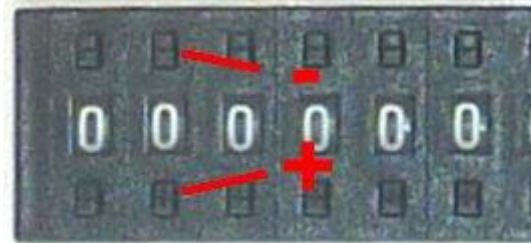

c. If you are making a remedy, place the blank remedy onto the right broadcast plate. This could be a be an uncharged dropper bottle containing 25% brandy and 75% water, a small vial of sugar pillules (typically used by homoeopaths) or a blank balm or cream (for skin conditions). It could also be a psychometry message typed or written on a piece of paper included in the remedy or in the broadcast e.g., "Stop Smoking" or "Stop Drinking Alcohol". Note that directional messages for self gain or evil can have karmic consequence, so it is advised to use messages with direction very carefully if at all, or to ensure that it is discussed with the client before broadcasting so that they are aware.

d. Set the the *Continuous/Transfer Only* switch to TRANSFER ONLY (Recommended) for a standard timed cycle of 24 seconds. You can alternatively use CONTINUOUS for an untimed always on function, but when you switch to continuous, the energize cycle will start so it is better to switch to continuous AFTER pressing Energize button (see [below](#)).



The duration of long-term broadcasting usually should not exceed 10 - 60 minutes. There is a separate indicator LED that indicates continuous broadcast is on.



It is suggested that one use Kinesiological testing, dowsing or intuition for the ideal duration and for making other selections. However you may choose to Broadcast Continuously (when making remedies) by Selecting "Transfer Only" or "With Harmonics". While there is no maximum time for a broadcast, the user needs to be aware that the longer the broadcast, the bigger the risk risk of the body acclimating (becoming used to the frequency rendering it ineffective). The skilled practitioner should use the sense pad, or other techniques such as kinesiology when determining the maximum broadcast time.

e. If making a homoeopathic remedy, set the potency knob to adjust the strength of the broadcast (6x lowest; 50M highest).





f. You can optionally add audio healing frequencies from any unit that has a 3.5mm headphone socket with *standard line level audio* output (e.g., an iPod, iPhone, mp3 player, radio, computer headphones outlet or a smart phone). The male to male 3.5 mm lead is used to connect your signal to the input on the rear of the unit marked B in the photo to the below. (Note: Standard Line Level Output is usually audio output suitable for headphones and must not exceed 1V RMS which can otherwise void warranty on the Hypertronic Pro. It is recommended that you check audio output specifications for the unit you are attaching *before* connecting).



- Adjust BODY knob for desired level of consciousness. As a guide, the number settings are as follows: 0 – Neutral, 1 – Physical, 2 – Emotional, 3 – Mental, 4 – Astral, 5 – Etheric, 6 – Celestial (Lower Spiritual) and 7 – Ketheric (Higher Spiritual). For Home Users, it is recommended that you leave this setting at 0. Zero is basically a pass-through, removing the use of any setting, so that it does not need to be part of a particular plan.



- Optional: Add a will power intention to your remedy using the sense stick pad. Remember to always get the permission of the targeted witness when using sense as you are subjected to the laws of karma if you broadcast an intention unknowingly to the target.



- Press the ENERGIZE button to complete a 24 second energize/broadcast. The yellow LED close to the voice switch will blink while energizing is continuing. Wait for the cycle to complete. If doing a broadcast, this length of time is all that is necessary. To stop a continuous broadcast, first remove the remedy (if there are any on the input or output plates) THEN switch POWER off. If you wish to bypass the 24 second timed energize, switch from Transfer Only to Continuous JUST AFTER pressing the Energize button.



- If you wish to add a multiple rates to your remedy, repeat the process and energize the same remedy (e.g., pillules) for each rate. The resulting remedy will then consist of a number of rates.



Caution: When adding several rates, you risk one rate interfering with another so use dowsing or intuition if you are intending to add multiple rates to the same remedy. As a general rule, a single rate is best, but you can add up to 5 rates if one does not interfere with the other.

---

### OTHER AVAILABLE OPTIONS

If you have your patient sitting with you, they may choose to apply the frequencies directly to them using the copper hand piece.



Connect the hand piece to port E shown below using one of the banana plug leads provided.



Ask your patient to hold the hand piece and then press the Energize button.

---

In circumstances where the witness plate or broadcast plates are too small, use the provided copper plate to get a larger surface area to work with.



Connect the copper plate to port A for a larger witness plate, or to port E for a larger broadcast plate.



### 3c. CREATING VIBRATIONAL REMEDIES

Use this procedure when using rates from one of the publications to create a vibrational remedy such as a homoeopathic, a flower essence etc


1. Zero everything by pressing the CLEAR button and wait for the process to complete.



2. Remove any voice recording by pressing the record button briefly once.




3. Set to DIRECT.

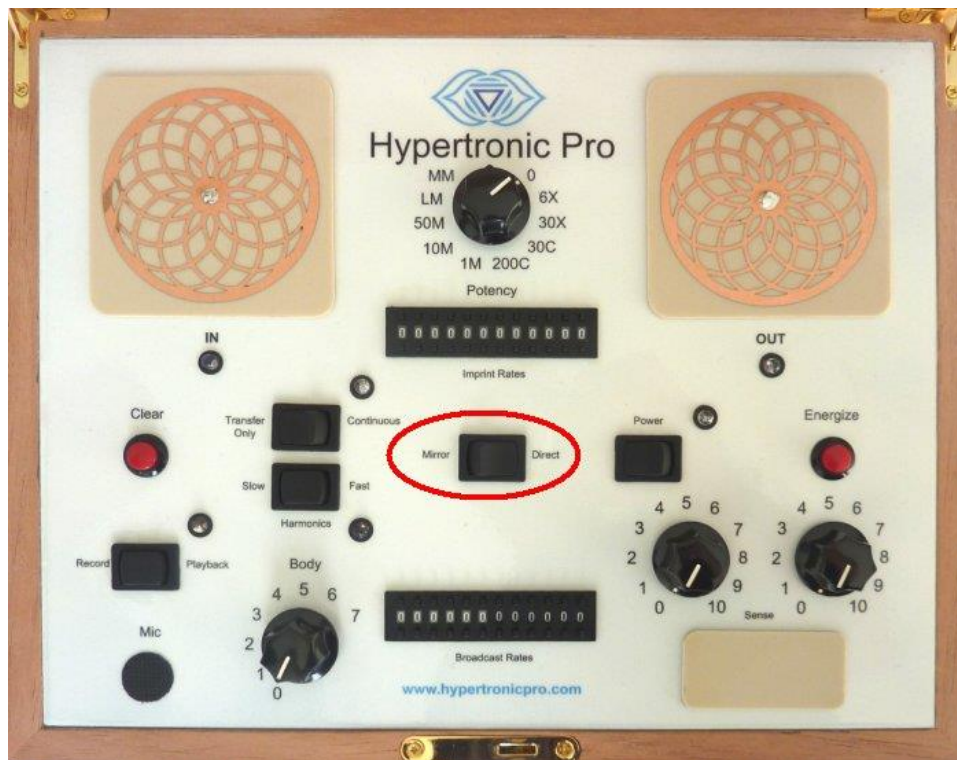


4. Consult the [reference guides](#) to determine the rate of the remedy that you are creating (click [here](#) to view the available guides). For homoeopathic remedies, input the rate in the upper rate bank: IMPRINT RATES.




For radionic remedies, enter the rate into BROADCAST RATES.

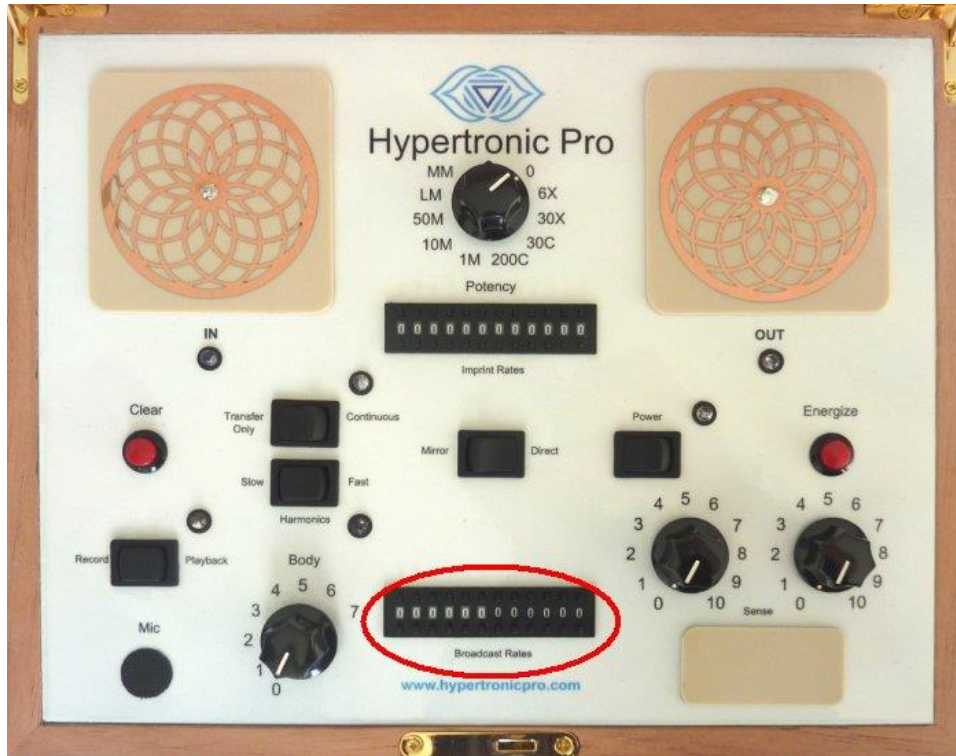

5. Always make sure numbers are entered from the right side. For example the Sulis guide says that the rate for producing a Typhoid vaccine is 61189991. It should be entered as 000061189991 as shown in the picture below and NOT as 611899910000.

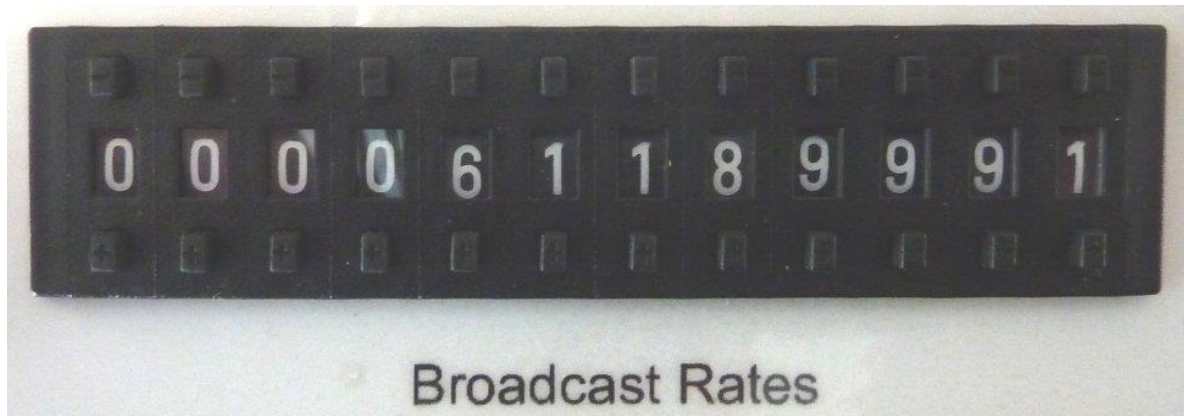

6. If making a homoeopathic remedy, adjust the POTENCY knob for desired potency.

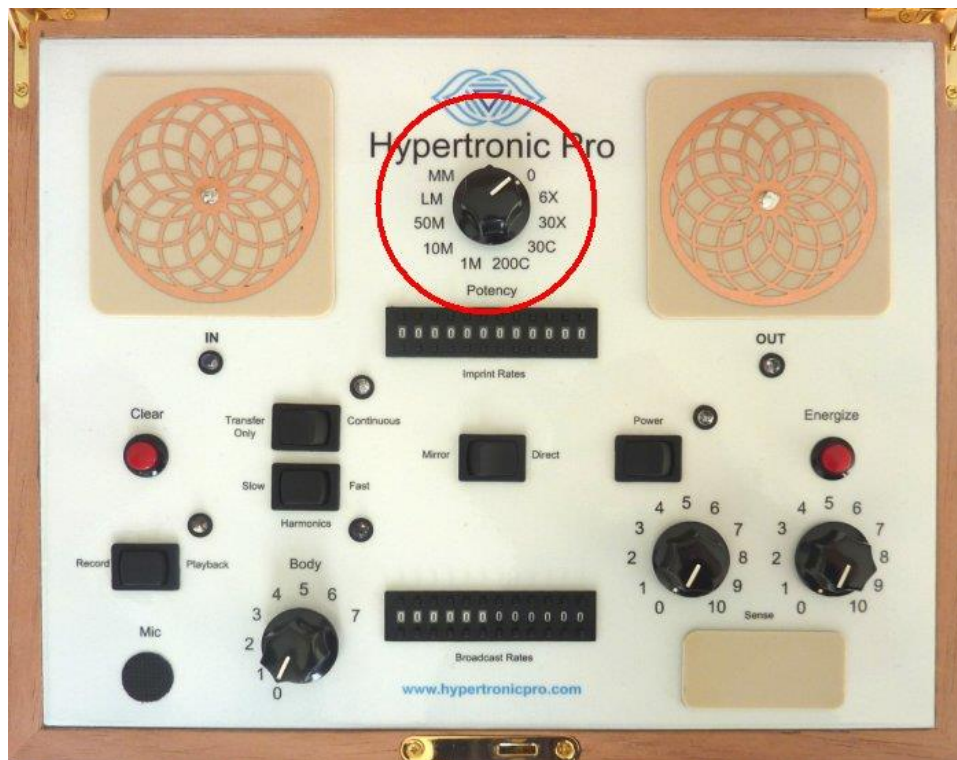

7. Place target (e.g., dropper bottle or pillules as described above) on broadcast plate on the right side of the unit.





8. Press ENERGIZE for timed operation. The energize process will take approximately 24 seconds to complete.



### 3d. COPYING VIBRATIONAL REMEDIES

All forms of vibrational medicine remedies (e.g., homoeopathics, flower essences, radionic and so on) can easily be copied using the following procedure.

1. Zero everything by pressing the CLEAR button and wait for the process to complete.



2. Remove any voice recording by pressing the record button briefly once.



- Place the remedy being copied onto the left witness plate, and the blank remedy onto the right broadcast plate.



- Set to DIRECT.



5. Ensure Imprint Rates and Broadcast Rates are set to zero.



6. Press ENERGIZE for timed operation. The energize process will take approximately 24 seconds to complete.



### Notes

- When using the INPUT plate for copying, the lower rate bank is still able to be used. This adds the possibility of a second rate/remedy to a vibrational imprint.
- Place WITNESS SAMPLE (and optionally any REMEDIES to include in the test) on the LEFT "IN" Plate -- AND if Making a Remedy -- Place Virgin Dropper Bottle w/ Distilled Water or Lactose Pellets on the RIGHT "OUT" Plate. Always ensure that glassware (e.g., 30-50mL dropper bottles, clean small glass jars etc) are used on the right hand plate when making remedies as plastic and other material containers are unsuitable.

## USING THE SENSE STICK PAD

The sense stick pad is an integral part of the Hypertronic Pro and it is used to harness will power of the user to the targeted witness (which could be a strand of hair, a photo etc which is on the witness plate). It can be used by advanced radionics therapists, or by those wishing to use their psyche as part of the remedy which they are creating. It is particularly useful in psychotronics. **If you prefer not to include the Sense option in your work, simply leave the 2 knobs set at zero.**



The stick pad is an optional tool for connecting operator mind and for tuning thoughts with reality for finer radionic adjustment. By gently stroking the surface of the small plate with a finger(s) (usually in direction towards the user) a change in the energy level can be felt on finger tips with a *sticking effect*. The 2 knobs are adjusted accordingly to fine tune the broadcast plate with intention and manifestation when needed.

Start with the 2 knobs set at zero. Focus your mind on the point that you are trying to will, and begin to turn the left knob clockwise. When you get the sticking effect, leave the knob in that position, then repeat the procedure on the right knob. You will then have 2 knobs at 2 different positions, containing the thought or manifestation being included in the broadcast or remedy. You are then ready to energize.



**Warning.** Always make sure that you have permission of the patient if adding your will power for a broadcast, which otherwise subjects you to the laws of Karma.

## Theory

Many people are confused by this divination method.

The stick pad within the Hypertronic Pro is a copper plate linked directly to the core of the manifest generator and the rate circuit. On top of this copper plate is a thin polymer layer.

While the stick pad primarily relies on the ideomotor response of the operator there may be a few more subtle energies involved in actually getting the stick. Ministry of defence research suggests that the low frequency natural electric fields, or static as it is commonly known is a manifestation in some degree of the fundamental energy of the universe termed orgone or chi.

When you use a stick pad which has a layer of plastic over the copper plate you are able to create a small amount of static by the rubbing process. It is within some of this static that the orgone energy resides, which can act as a carrier for intention and the radionics signals being output from the Hypertronic Pro.

It is a combination of these factors which make the stick pad a formidable dowsing device. It is also the cause of why many people find the stick pad difficult to get used to and opt instead for a standard pendulum. Because the stick pad is producing a combination of energies an experienced pendulum dowser will have trouble overriding their natural ideomotor response to a pendulum. This act is not conscious but resides within the subconscious.

The key to using a stick pad is to let all preconceptions fly out of the window and trust the reactions you are getting from the rubbing plate.

The reaction or *stick* manifests uniquely for each and everyone of us. For some it will appear as if their finger is getting heavier, for others it will manifest as sticky finger and your finger will be pulled due to friction.

Having just mentioned fingers, it is worth noting that no specific finger or thumb is recommended over the others, just use which ever you feel comfortable with.

It really is worth giving the stick pad a go. If at first you don't succeed then keep on trying.

## 4. USEFUL RADIONIC RATE GUIDES FOR USERS OF THE HYPERTRONIC PRO

We have made a selection of Radionic Rates Guides available for free download at <http://www.hypertronicpro.com/radionic-references>.

The guides are from some of the most respected researchers in the field of radionics. Please note however that we do not necessarily endorse the rates, frequencies or the work of other researchers presented in the guides. They are presented here purely as a matter of convenience for users of the Hypertronic Pro.

The rate guides available include;

- [Sulis Remedy Maker Standard Rates](#)
  - [Kelly Radionic Rates](#)
  - [Materia Medica of Homoeopathic Formulas by Bruce Copen](#)
  - [Homoeopathic Rates Listing by Bruce Copen](#)
  - [Radiobiology Therapy by Bruce Copen](#)
  - [Organs and Symptoms Rates Book](#)
  - [Copen Rates for Agriculture, Herbal and Flower Essences](#)
- [Applied Radionics](#) A training guide in Radionics by Kelly Research Technologies (KRT). Note: The Applied Radionics book uses KRT radionics hardware in its presentation. KRT are not associated with the Hypertronic Pro; all the same we see it is a useful guide in learning and understanding the science of radionics.

## 5. CLEANING AND CARING FOR YOUR HYPERTRONIC PRO

When the Hypertronic Pro is not in use, it is recommended that you keep the lid closed and locked. There are 2 keys provided with the Hypertronic Pro to lock the box. This ensures that no one but you can use the instrument, and it also ensures that the plates are kept clean from dust. When using the Hypertronic Pro, it is essential to ensure that no fingerprints make their way onto the plates or onto any of the witness samples. If your fingerprints are there, then you will become part of the radionic circuit, and will receive targeted transmission of frequencies in a broadcast.



### Cleaning the Plates on the Hypertronic Pro

lacquer.

If you accidentally touch the witness or broadcast plates, or if they need cleaning please use a clean damp cloth to wipe them over. Ensure that there are no fibers remaining on the plates after you have finished wiping. The plates are coated with a coat of lacquer to prevent oxidation, so it is important NOT to use any cleaning agents which could otherwise disturb the

### Cleaning the Extendable Accessory Plate

The Extendable Plate is made from an uncoated copper, and has a plastic lining on the back with plastic feet. Over time the copper surface may tend to tarnish. You can clean the accessory plate with alcohol such as methylated spirits (preferred as it will evaporate and leave no residue) or even acetone. Ensure that no residue remains on the plate which could otherwise affect readings or broadcasts.

It is recommended that you store the plate in the plastic bag in which it comes while it is not in use for maximum protection.



### Cleaning the Hand Held Copper Piece (Must always be cleaned between sessions)

It is important to clean the hand held copper piece every time after a patient has held it, as their fingerprints could create a targeted broadcast the next time another patient contacts the piece (i.e., the previous patient will receive a broadcast of the frequencies intended for the next patient without the unit being cleaned). The hand held copper piece can be cleaned in the same way that the accessory plate is cleaned. Alcohol such as methylated spirits is the preferred method. It is recommended that you store the hand piece in a resealable plastic bag while it is not in use for maximum protection.



## 6. HYPERTRONIC PRO WARRANTY

Natures Energies Health Products warrants to the original consumer/purchaser (herein after called "the owner") that the Hypertronic Pro (herein after called "the product") shall be free from faults, as well as defects in material and workmanship **for a period of twelve (12) months** from the date of the original purchase subject to the conditions stated herein.

### **IF SERVICE IS REQUIRED DURING THE WARRANTY PERIOD**

Where service is required during the warranty period, these repairs would be carried out with no charge to the owner, subject to the conditions specified herein.

If up until 72 hours after receiving the product, there is failure in the product, then the manufacturer is responsible for any transportation and insurance costs to and from our contracted engineer in U.S.A should the product require being repaired. The manufacturer has liability for any freight or transportation damage during transit in these circumstances.

After 72 hours of receiving the product the owner is responsible for any transportation and insurance costs to and from our contracted engineer in U.S.A, should the product need to be repaired. The owner in these circumstances has liability for any freight or transportation damage during transit.

Should our contracted engineer in USA determine that the product is not faulty, or that damage is outside warranty conditions (*See When this warranty does not apply below*), then the owner is responsible for the cost of having the product returned to them, and no costs for transport (as is the case for failure within 72 hours) will be paid to the owner. In these circumstances, the assessment made by our contracted engineer is final. The owner may request in this case for repairs to proceed, but is responsible for labour and part costs, as well as transportation and insurance.

If after the 12 month warranty period has expired repairs are required, costs for labour and parts will be charged to repair the product.

### **WHEN THIS WARRANTY DOES NOT APPLY**

This warranty does not extend to accessories or defects or injuries caused by or resulting from causes not attributable to faulty parts or manufacture of the product, including but not limited to, defect or injury caused by or resulting from misuse, abuse, neglect, accidental damage, improper voltage, liquid spillage, or vermin infestation.

The warranty also does not apply where audio hardware with output exceeding 1V RMS has been connected to the audio input of the product, resulting in damage. Generally hardware with audio output for headphones has *standard level audio output* which is 1V RMS output, but it is up to the owner to check with manufacturer specifications before connecting to the product.

### **CONSUMER PROTECTION LAWS**

This Warranty is in addition to and does not in any way affect your rights under the Trade Practices Act 1974 (Australia). For owners who are covered by consumer protection laws or regulations in their country of purchase or, if different, their country of residence, the benefits conferred by this

warranty are in addition to all rights and remedies conveyed by such consumer protection laws and regulations.

Some countries, states and provinces do not allow the exclusion or limitation of incidental or consequential damages or exclusions or limitations on the duration of implied warranties or conditions, so the above limitations or exclusions may not apply to you. This warranty gives you specific legal rights, and you may also have other rights that vary by country, state or province.

This Limited Warranty is governed by and construed under the laws of the country in which the product purchase took place. Apple, the warrantor under this Limited Warranty, is identified at the end of this document according to the country or region in which the product purchase took place. *Note:* Please retain your purchase invoice, as this should be produced to validate your warranty claim.

## 7. HYPERTRONIC PRO DISCLAIMER

Cyberlab Systems Pty Ltd T/As Natures Energies Health Products (hereinafter "Natures Energies") means to include any parent, employee, contractor, and/or representative or any other rights holder, officer, affiliate, and member of Natures Energies).

### ***Hypertronic Pro***

The Hypertronic Pro is not a diagnostic tool for orthodox medical conditions. While we provide a number of downloadable references with radionic rates which can be programmed into the Hypertronic Pro, and while these rates have disease pattern labels, organs references and so on, they are simply intrinsic data field correlations based on the observations of the pioneers in this field, and must not be misconstrued as cures to medical conditions. Natures Energies does not necessarily endorse the rates, frequencies or work of any radionics researcher presented in the radionics references, or other guides that are available in the field of radionics. The Hypertronic Pro is not intended for the diagnosis, prevention, vaccination, treatment, cure or mitigation of any disease in humans or animals. It is not designed to affect the structure or function of any system in the body. If you have a health-related condition that requires medical attention, always consult with a licensed health care professional.

Radionic Instrumentation is not approved by the United States of America food and Drug Administration (FDA) for use by health care professionals or vets in their practice.

### ***Natures Energies Products in General***

Natures Energies products are sold as experimental devices and artistic creations, for learning, self-improvement, spiritual development, and simple relaxation, and are not offered for the treatment or cure of any disease. There is no guarantee of effectiveness for any of these products. No statement contained in this manual, and no information provided by Natures Energies, should be construed as a claim or representation that these products are intended for use in the diagnosis, cure, mitigation, treatment or prevention of disease or any other medical condition. You should not use any of the information for diagnosis or treatment of any health problem or for prescription of any medication or other treatment. You should not stop taking any medication without first consulting your physician. The information contained in this manual is deemed to be based on reliable and authoritative report. However, certain persons considered experts may disagree with one or more of the statements contained here. Natures Energies assumes no liability or risk involved in the use of the products described here. We make no warranty, expressed or implied, other than that the material conforms to applicable standard specifications.

Natures Energies does not accept any responsibility for the accuracy of the information or the consequences arising from the application, use, or misuse of any of the information contained herein, including any injury and/or damage to any person or property as a matter of product liability, negligence, or otherwise. No warranty, expressed or implied, is made in regard to the contents of this material. This material is not intended as a guide to self-medication. The reader is advised to discuss the information provided here with a doctor, pharmacist, nurse, or other authorized healthcare practitioner and to check product information (including package inserts) regarding dosage, precautions, warnings, interactions, and contraindications before administering any drug, herb, radionics tool, supplement or product discussed in this manual.

Natures Energies products are for the sole purpose of educating people about intuitive abilities and environmental energies, and are for general information purposes only. The listing of a person, organization or other entity in any part is for convenience only and in no way implies any form of endorsement of the information, products, or services provided by that person, organization or other entity.

All concepts, procedures, and technology described herein are speculative, not necessarily approved by any Government agency, and may be hazardous to susceptible or unqualified persons. In all instances, no diagnostic or therapeutic claims are made or implied. Please consult your licensed physician for medical advice. It is a condition of viewing this that you read and agree to the full disclaimer. Thank you for your understanding.

The products and the claims made on or through Natures Energies products, emails, publications, or advertisements have not been evaluated by the United States Food and Drug Administration and are not approved to diagnose, treat, cure or prevent disease.

Consult a physician before using these products if you have any medical condition whatsoever, or if you have or suspect you might have a health problem, or if you are pregnant, or if taking any kind of medication. In accordance with FDA regulation, we do not make any therapeutic claims regarding the health benefits of any products. If you have any medical problems, please be advised to contact your doctor.

No promises, guarantees or warranties, whether stated or implied, have been made that you will produce any specific result as a result of purchasing our products, or using information from our website/email. Information may contain technical inaccuracies or typographical errors. Information may be changed or updated in our web site without notice.

This manual contains information which is for information only. It does not constitute medical advice and makes no warranties as to fitness for any particular purpose. Users should consult a health professional about any information presented here to determine its suitability.